


# FREEDOM FROM REPROCESSING DISPOSABLE ACCESSORIES FOR ESOPHAGEAL DILATORS

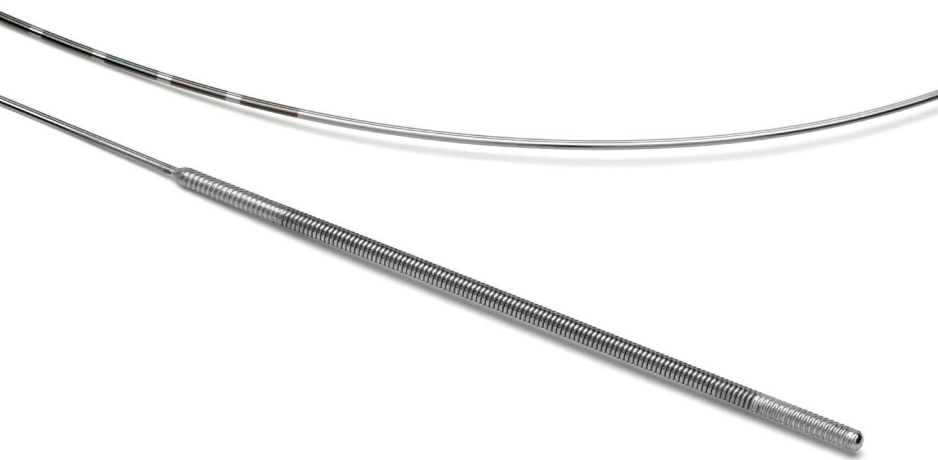

Repeated use and reprocessing of reusable guidewires and cleaning brushes can result in worn, frayed, bent or otherwise damaged devices.


The use of disposable guidewires and disposable cleaning brushes can reduce the risk of device damage as well as the potential cross-contamination from using reprocessed accessories with reusable polyvinyl dilator systems.

The Single-Use Marked Spring Tip Guidewire and Dilator Cleaning Brush are for use with American and Savary dilators.

## SPECIFICATIONS

### MARKED SPRING TIP GUIDEWIRE STERILE

Order Number	Description	Length (cm)	Package Units
DG25111	Single-Use Marked Spring Tip Guide Wire for Esophageal Dilators	210	10/Box

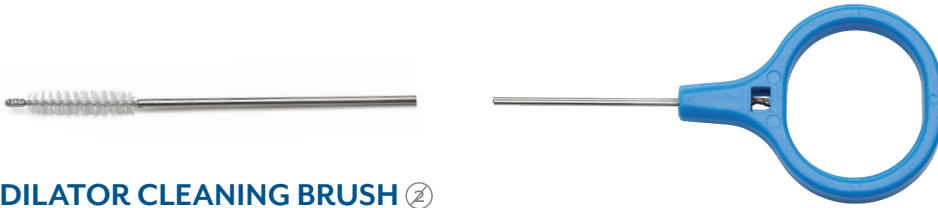

### DILATOR CLEANING BRUSH

Order Number	Description	Package Units
CB62411	Dilator Cleaning Brush, 3 mm for reusable American and Savary Dilators	10/Box

### CAN'T FIND IT?

Additional items may be available. Contact us if you can't find what you need.